

Width of Chair between the arms, 21 inches.
Highest position, 32 inches; lowest position, 22 inches.


<i>Prices :</i>		£	s.	d.
Chair in Green or Maroon Plush, as illustrated	23	10	0
" " with Spittoon Holder to fit on the arm,				
Nickelled Spittoon and Blue Glass Funnel	24	10	0
" with Adjustable Attachment, as shown on page 41,				
including Allan's Table and Lamp, Glass Tumbler,				
Nickelled Spittoon and Blue Glass Funnel	29	15	0
Case and Packing extra	1	0	0
Full amount allowed for the case if returned, carriage paid, and in good condition.				

Parts separately :

Adjustable Chair Attachment, as shown on page 41, complete	6	5	0
Spittoon Holder to fit Arm of Chair, Nickel-plated	0	15	0
Spittoon (Ash's), Nickel-plated, to hold 3 pints	0	13	0
Blue Glass Funnel for Spittoon	0	2	0
Ruby	0	3	0

DENTAL CHAIR.

(FIG. XXVII.)

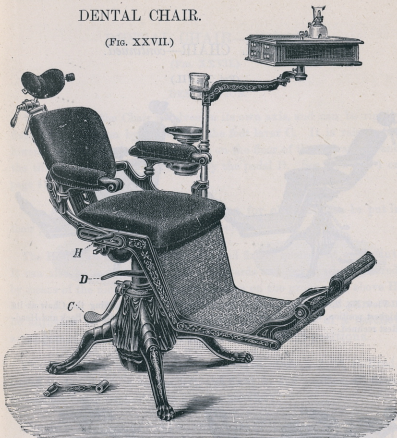

View No. 1.—Chair complete, with Attachment.

Width of Chair between the arms, 21 inches; highest position of seat, 33 inches; lowest position, 22 inches; highest position of head-rest, 61 inches; lowest position, 26 inches; lowest position of head-rest when the chair is tilted as in view No. 5, 26 inches.

For usefulness, style, and durability, this Chair is one of the best and cheapest that has been introduced, and we can strongly recommend it. The different positions in which it is illustrated represent a few of the numerous movements which it possesses.

Like Chair Fig. XXIII., shown on page 38, it is upholstered and finished in the best manner, the iron frame-work being nicely japanned, tastefully relieved with ornamentation, and all the bright parts nickel-plated.

For description and prices, see page 43.

DENTAL CHAIR—*continued.*


(FIG. XXVII.)




View No. 2, showing the Chair at its highest position, with the Back and Head-Rest reclined.



View No. 3, showing the Chair at its highest position, with the Back and Head-Rest upright.



View No. 4, showing the Chair at its highest position, with the Body tilted to the fullest extent.




View No. 5, showing the Chair with complete Attachment. In this illustration the lowest position is given, and the Body is tilted to the fullest extent.

MORRISON'S DENTAL CHAIR,

WITH

IMPROVED TILTING LEVER E, Suggested by Mr. CLAUDE ROGERS.



Highest position, 40 inches; lowest, 15 inches; width of seat between the arms, 19 inches.

Considering its Strength, Quality, and Workmanship,
we claim that this is the cheapest and best
Morrison Chair at present made.

WIRE SPRING SEATS FOR DENTAL CHAIRS.

(INTRODUCED BY DR. HENRY WESTON.)

Fig. 1.




Fig. 1 shows the wire seat ready for receiving a layer of stuffing and the cover of plush or leather.

Fig. 2.




Fig. 2.—Portion of Dental Chair showing part of the wire seat uncovered for the purpose of exhibiting its form in position.

HOSPITAL CHAIR.



Highest position, 27 inches; Lowest position, 16. Width of Chair between the arms, 18 inches. Length of Base, 35 inches; width of Base, 16 inches.

This Chair is in general use at the Dental Hospital of London. It is substantially made of polished wood, the combined back and head-rest being plainly covered with American cloth, and will stand the hard wear and tear to which it may be subjected in a public institution.

It is fitted with folding Foot-Rest, movable iron Bracket, and plain oak Instrument Table, as shown in the engraving.

The Body slides up or down the frame of the Chair, and rests in one or other of the iron slots designed to receive it. These slots are placed at a distance of three inches from each other. There is a locking lever at the back which firmly secures the body in any of the slots in which it is placed.

The Back and Head-Rest, which are made in one piece, can be raised or lowered as under:

When the Body is raised to its highest position and the Back is fixed at its lowest, the distance from the seat to the top of the Head-Rest is only 18 inches.

When the Body is fixed in its lowest position and the Back is drawn up to its full height, the distance from the Seat to the top of the Head-Rest is 31 inches.

It will be seen from these measurements that the Chair has a working range of 13 inches, and that it is suitable for patients of almost any stature.


		£	s.	d.
Price complete, as illustrated	..	8	10	0

HOSPITAL CHAIR.




	s.	d.
Chair as illustrated, supplied to the London Dental Hospital	190	0
Chair (Mr. Owen's) Improved—see page 44 of our 1886 Catalogue—in Birch-wood, with Footstool attached, and Head-Rest covered in Leather, as supplied to the Liverpool Dispensary	325	0

Fig. 2.



Footstool in Walnut, 20 inches long by 16½ inches wide, with two steps covered with carpet, which can be raised or lowered, and fixed at different elevations by means of a spring ratchet. Highest step 12 inches, which can be raised to 15 inches; lowest step 5 inches, which can be raised to	s.	d.
7 inches (Fig. 2.)	42	0
" .. not covered	34	0
" .. without ratchet action	30	0

ASH'S ADJUSTABLE STOOL.



This Stool has a range of $8\frac{1}{2}$ inches, the lowest position being $22\frac{1}{2}$ inches, and the highest position 31 inches. We have introduced it in response to a demand for a much lighter article than Lyons' and Greenfield's Stools. As the total weight is only $18\frac{1}{2}$ lbs. it can easily be lifted with one hand and placed in any desired position. It is elegant in appearance, the Seat being upholstered in green or maroon plush or leather, the Pillar nickel-plated, and the Base japanned black, relieved with ornamentation.

The Seat is raised and lowered by means of a screw, while the backward and forward movement is controlled by a nickel-plated foot-lever at the Base, which can be worked while sitting on the Stool either with the right or the left foot.

Price, in Green or Maroon Plush, or Leather .. $\begin{matrix} \text{£} & \text{s.} & \text{d.} \\ 2 & 10 & 0 \end{matrix}$


FINGER BOWLS.

FOR THE OPERATING ROOM. In Blue, Green, or Ruby-coloured Glass.

Prices :						s.	d.
In Blue Glass	each	1	0
„ Green „	1	0
„ Ruby „	1	8

DENTAL CHAIR.

(FIG. XXVL)



Width of Chair between the arms, $19\frac{1}{2}$ inches; highest position, $25\frac{1}{2}$ inches;
lowest position, $20\frac{1}{2}$ inches.

This is the cheapest iron Chair which has yet been introduced to the Profession. It is strong and durable, simple in construction, and well adapted for general purposes.

Some idea of its usefulness may be gathered from the following description:—

The **Head-Rest** can be raised or lowered, depressed or turned backwards, moved to the right or left, and fixed in any position. In shape it is one of the most convenient in use. It can be had with an Arm-Support, which is not shown in the illustration, at an extra cost of 10s.

The **Back** can be fixed upright or reclined by means of the ratchet movement shown below the back of the seat. The lower portion of the